

IsoMist[®] Temperature Controlled Cyclonic Spray Chamber With Extended Temperature Range

The IsoMist programmable temperature controlled cyclonic spray chamber features an improved thermodynamic design providing an extended temperature range and faster cool-down, so your ICP is ready to go sooner.

The IsoMist is a compact, convenient and maintenance-free temperature controlled sample introduction system for all ICP's.




Improved Analytical Stability with Precise Temperature Control

On the IsoMist, the spray chamber temperature is accurately controlled through an improved thermodynamic design using a multi-stage peltier device. The spray chamber temperature is settable in 1°C increments from -25°C to 80°C guaranteeing optimum conditions can be used for any application. The improved cooling efficiency of the new dual-stage peltier design means it is ready, sooner and the cool-down time is reduced.

Reduce Oxide Interferences in ICP-MS

Using the IsoMist spray chamber at sub-ambient temperatures on an ICP-MS, the sample is cooled, less water vapor is transferred to the plasma resulting in lower oxide formation and reduced polyatomic (ArO, ArOH) interferences (*Figure 1*). Less oxides in the plasma mean fewer interferences, improving accuracy and detection limits.

Figure 1. Effect of IsoMist Temperature on ICP-MS Oxide Ratio. Data Courtesy of David Jones, ALS Chemex

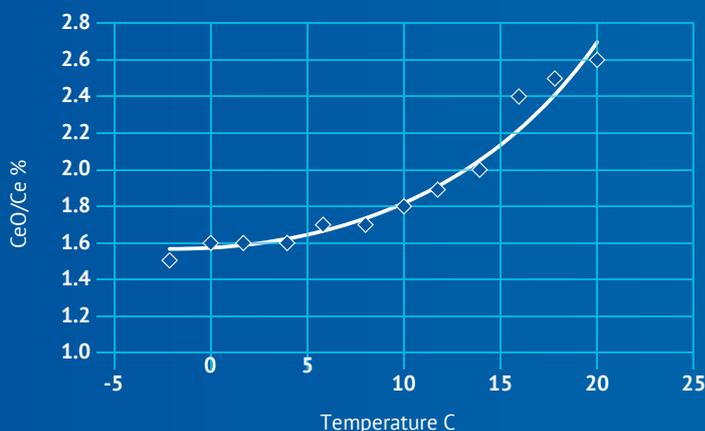

Perfect for Naphtha and Gasoline Analysis

For volatile solvents, a lower sample introduction temperatures reduces nebulization efficiency avoiding quenching of the plasma from solvent over-loading (see *Figure 2*). Now with a minimum operating temperature of -25°C , analyzing volatile organic solvents such as naphtha and gasoline by ICP is even easier.


Figure 2. Reproducibility results for undiluted naphtha at -10°C (measurements at 90 minute interval)

	Conc, ug/L	Conc, ug/L
Cd	57	55
Cr	31	32
Cu	35	33
Fe	24	23
Mn	11	12
Ni	589	517
Pb	451	424
Sn	216	213
Ti	22	22
V	107	104

Improve Analytical Stability with Constant Spray Chamber Temperature

Fluctuations in the lab temperature affects sample viscosity and nebulization efficiency. Maintaining the sample introduction system at a constant and stable temperature improves analytical reproducibility, enhances throughput and lowers operating costs by reducing the need to re-run samples when a calibration verification check standard (see *Figure 3.*) drifts outside the acceptable upper or lower limits.

Figure 3. Effect of constant temperature on signal stability

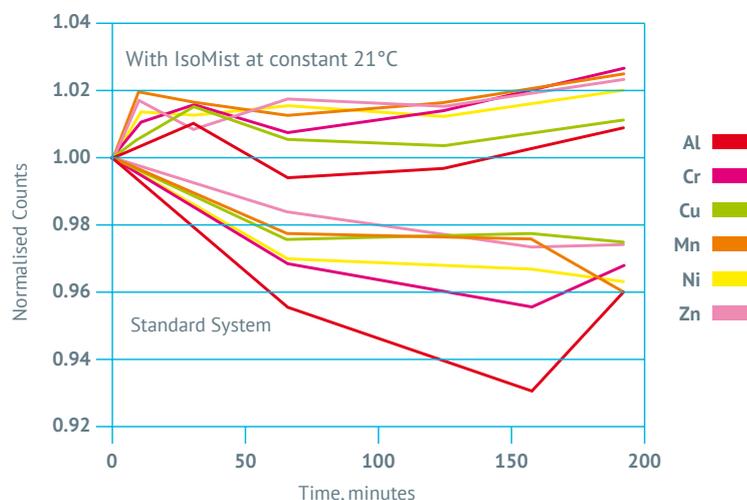

Elevated Sample Introduction Temperatures Enhances Sensitivity

The sensitivity for many analyses can be enhanced by operating the spray chamber at elevated temperatures - especially important for limited sample volumes. Heating the spray chamber also helps with the analysis of viscous samples such as lubricants and edible oils.

Easy to Use Software

For maximum convenience, the IsoMist can be controlled from a PC via USB or Bluetooth wireless interface. The spray chamber temperature can be monitored during an analytical run with time vs temperature plot on your PC screen.



Asia Pacific
 6 Central Boulevard
 Port Melbourne VIC 3207
 Australia
 +61 3 9320 1111
 enquiries@geicp.com

Americas
 31 Jonathan Bourne Drive
 Unit 7, Pocasset, MA 02559
 USA
 508 563 1800
 geusa@geicp.com

Europe
 Friedenbachstrasse 9
 35781 Weilburg
 Germany
 +49 6471 3778517
 gegmbh@geicp.com

Application Flexibility and Superior Design Innovation


The IsoMist incorporates Glass Expansion's proven Glass Twister cyclonic spray chamber design. A Quartz Twister and HF resistant, high-purity PFA Tracey design is also available upon request.. All of which are easily interchangeable, allowing for application flexibility should sample matrices change. All of Glass Expansion's cyclonic spray chambers, including the IsoMist feature the Helix CT interface. The Helix CT fitting is completely inert and carefully designed to fix the depth of penetration and torque of the nebulizer seal so that the aerosol produced is optimal. The Helix interface is also the only true zero-dead volume nebulizer/spray chamber interface providing unmatched washout efficiencies. These design innovations have provided Glass Expansion spray chamber sensitivity gains, reduced washout times and reduced matrix effects not possible with other spray chambers.



**Glass Twister Spray Chamber
with Helix CT**
P/N 21-809-3186



**Quartz Twister Spray Chamber
with Helix CT**
P/N 21-809-3192

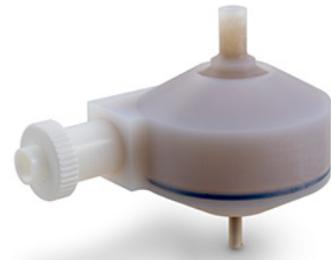

**PFA Tracey Spray Chamber
with Helix CT**
P/N 21-809-2985

Elegant, Ergonomic and Compact

The IsoMist is an elegant, compact, stand-alone system manufactured from materials resistant to attack from acids and solvents commonly used in ICP analysis. By using a peltier to maintain the spray chamber temperature, the messy, noisy and high-maintenance refrigerated circulating baths used with jacketed spray chambers has been eliminated. The compact design means all IsoMist Programmable Temperature Controlled Spray Chambers are compatible with virtually any ICP-OES or ICP-MS.

Contact enquiries@geicp.com for details on connecting IsoMist to your specific ICP-OES or ICP-MS model.



Asia Pacific

6 Central Boulevard
Port Melbourne VIC 3207
Australia
+61 3 9320 1111
enquiries@geicp.com

Americas

31 Jonathan Bourne Drive
Unit 7, Pocasset, MA 02559
USA
508 563 1800
geusa@geicp.com

Europe

Friedenbachstrasse 9
35781 Weilburg
Germany
+49 6471 3778517
gegmbh@geicp.com